


Microvette® 100/200

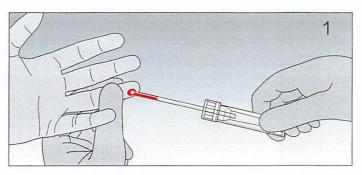


1) Collect blood with the assembled End-to-End 100ul or 200 ull capillary. For collection, best results are achieved if the Microvette® is held in horizontal or slightly inclined position.

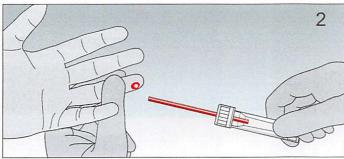

Collection is complete when the End-to-End capillary is entirely filled with blood.

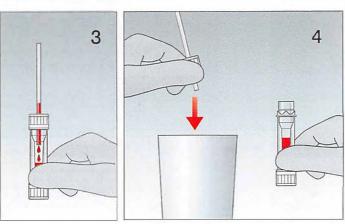

- Hold the tube upright to allow the blood to flow from the capillary into the Microvette[®].
- Turn the cap to remove and discard the preassembled capillary as one unit.



- 6
- Remove the cap from the base and seal the Microvette[®] ('click' position).
- Mix sample thoroughly by inverting the Microvette[®].

All patient blood specimens should be treated with standard precautions. Always wear gloves!



Your Distributor is: Braintree Scientific, Inc. PO Box 850498, Braintree, MA 02185 781-917-9526

Email: Info@braintreesci.com Web: www.braintreesci.com